

Sequencing Quality Control Report

Genomics Unit

June 26, 2014

1 Flowcell Information

Flowcell BC4WCWACXX
Run Start 2014-06-19
Read Length 50 single end
HiSeq Sequencing Kit Truseq v3


Sequencer Software HiSeq Control Software 2.0
Gerald version 1.8

2 Samples Information


LabID	Name	Index	NumberOfReads
7299	K27	CGATGT	43649998
7300	IgG	CAGATC	58867511
7301	IN	GTGAAA	78021280

3 Quality Plots

Sample 7299: K27

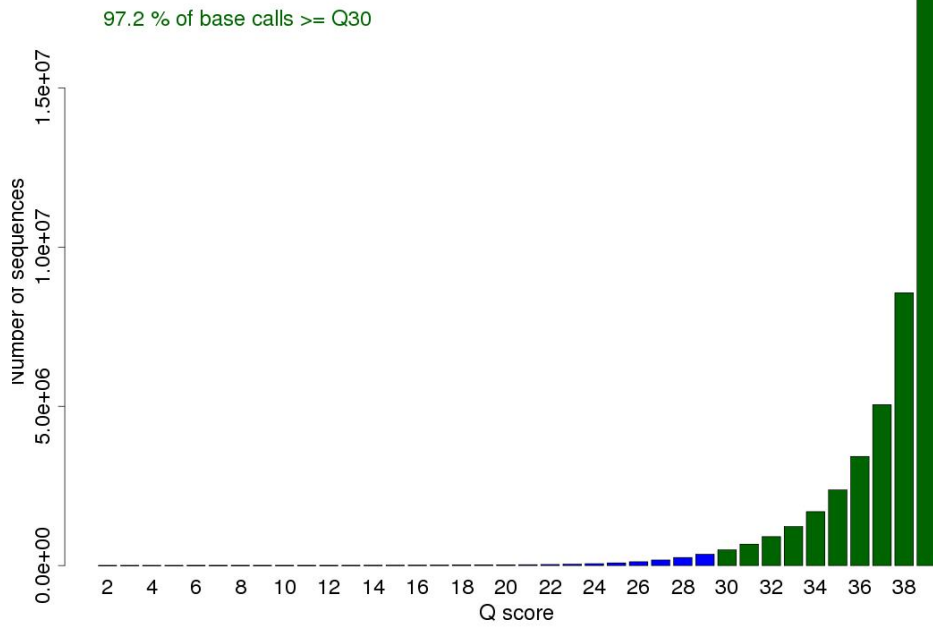

Sample 7300: IgG

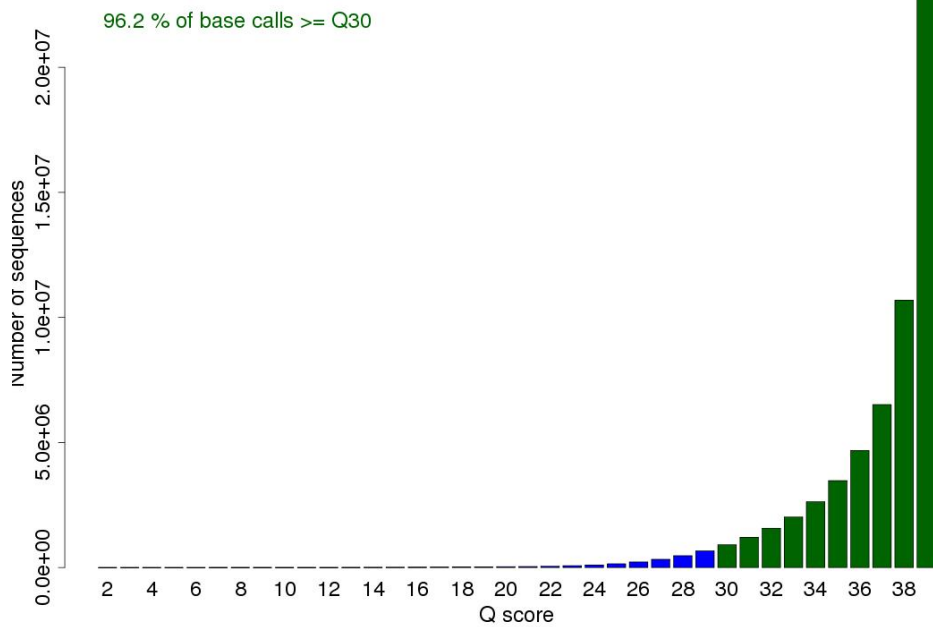

Sample 7301: IN

