

Sequencing Quality Control Report

Genomics Unit

July 10, 2014

1 Flowcell Information



Flowcell AC48V7ACXX
Run Start 2014-07-04
Read Length 50 paired end
HiSeq Sequencing Kit TruSeq v3

Sequencer Software HiSeq Control Software 2.0
Gerald version 1.8


2 Samples Information

LabID	Name	Index	NumberOfReadPairs
7339	ATAC lib B	TAAGGCG	41401470
7340	ATAC lib 18	CGTACTA	43978682
7341	ATAC lib d1	AGGCAGA	41715991
7342	ATAC lib d2	TCCTGAG	42317755
7592	ATAC Lib E14	GGA CTCC	21269679


3 Quality Plots

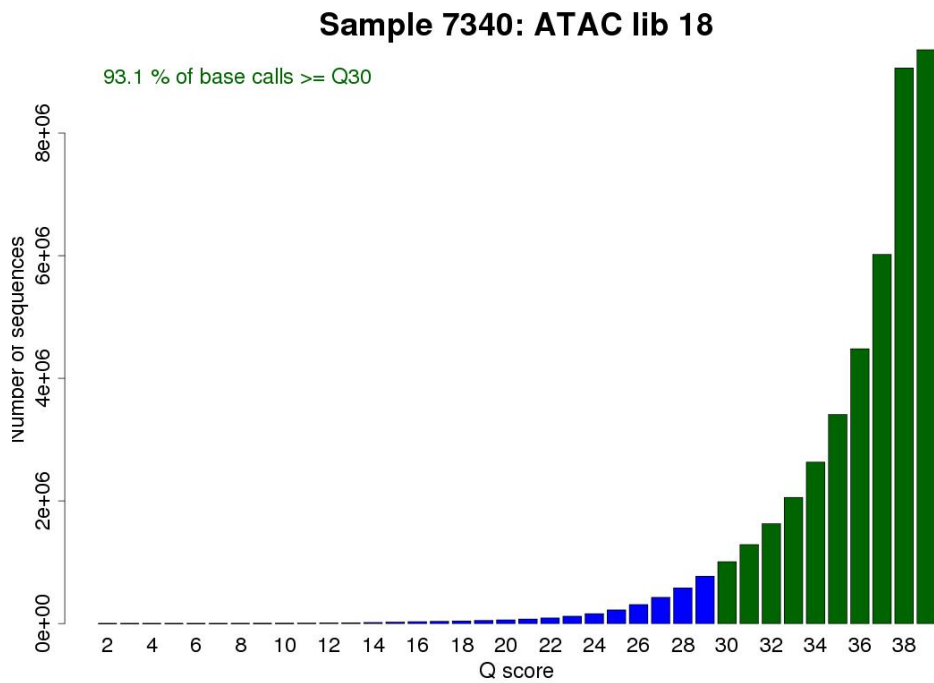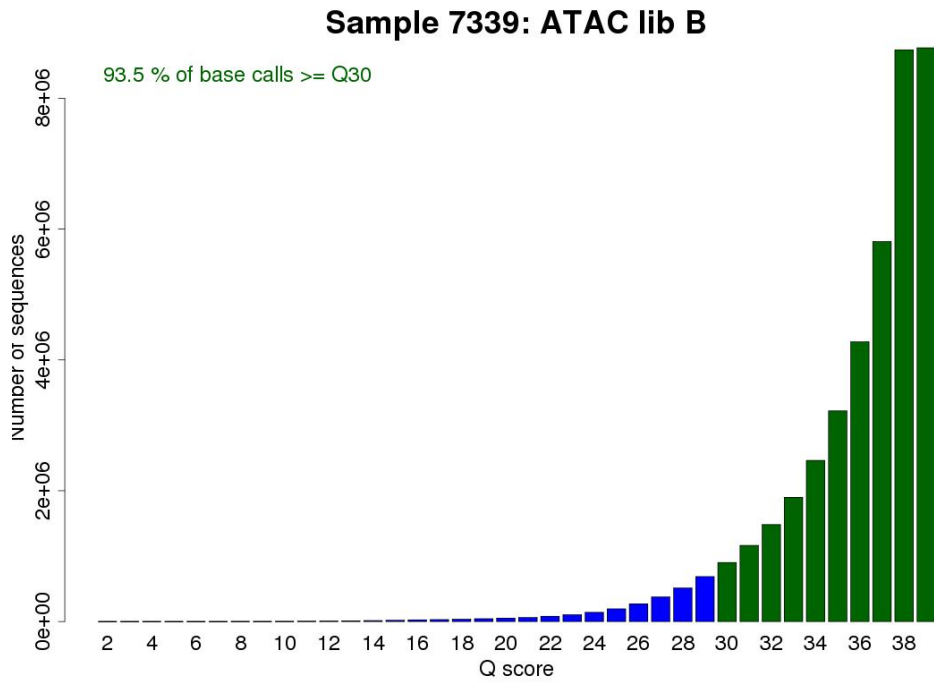

Sample 7341: ATAC lib d1

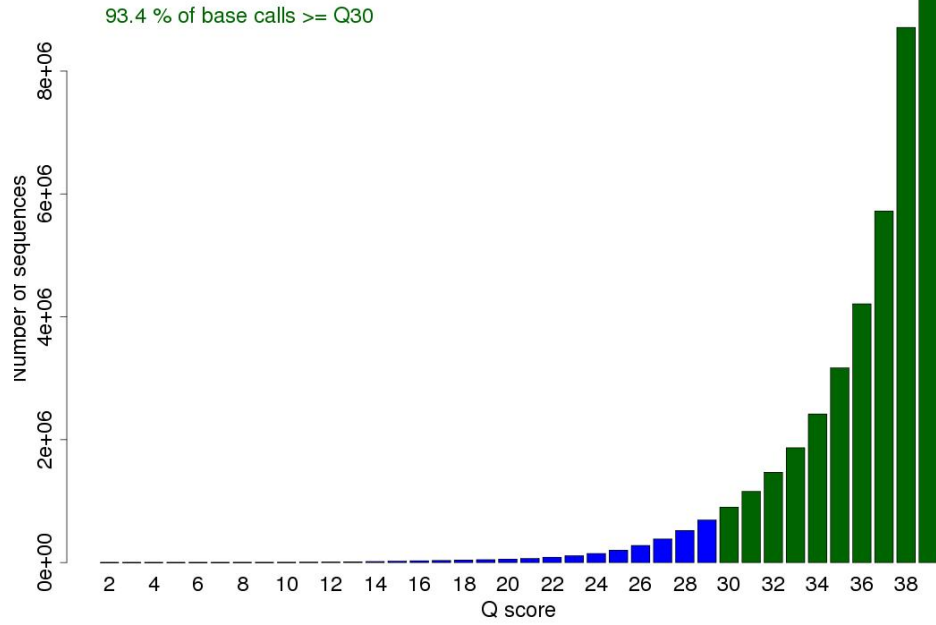

Sample 7342: ATAC lib d2

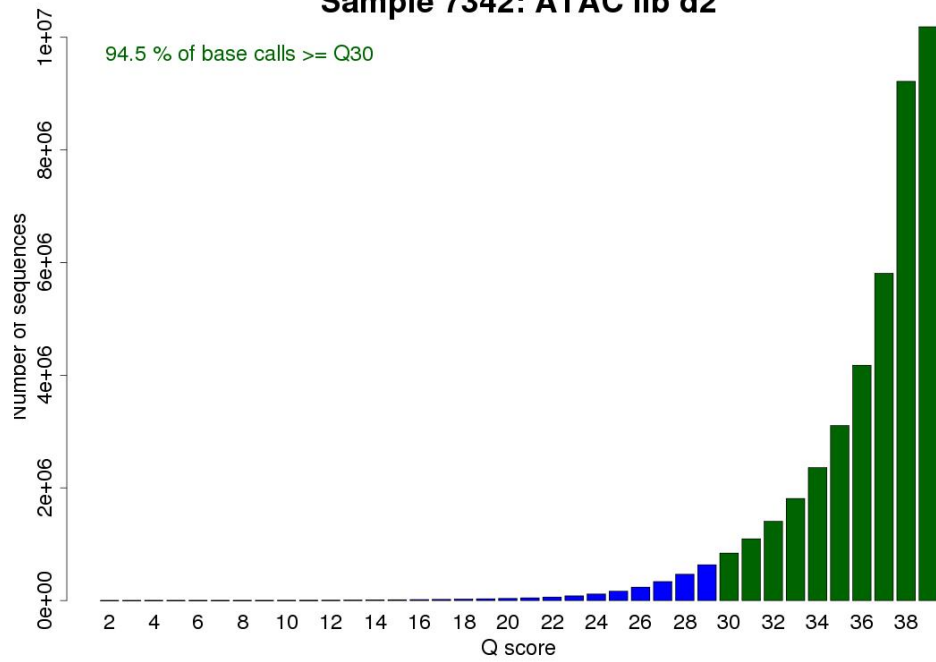

Sample 7592: ATAC Lib E14

